CONFORM®
Med.Luftkissen-Systeme

Conform Air Cushions

Operating Instructions

Remove the Conform cushion from its packaging. Inspect the product to ensure that there are no parts which are missing or damaged.

Parts include:
Cushion, Cover, Pump, User Manual

Optional Part which can be ordered separately:
Coverplate

Turn the air valve anti-clockwise to open.
Attach the pump tubing to the cushion valve.
Inflate the cushion until it begins to arch.
Close the air valve by turning it clockwise.

Adjustment

Seat the patient and open the air valve to deflate the cushion so that the patient comfortably sinks, however ensuring that their bottom doesn't touch the base of the cushion.
To ensure the cushion has been set correctly, ensure you are able to insert your hand between the patients bottom and the base of the cushion. The distance between the deepest point of a sitting person (usually the ischial tuberosities) and the base of the cushion should be approximately ¾ of an inch or 2 cm.

Cushion and Cover

Pump

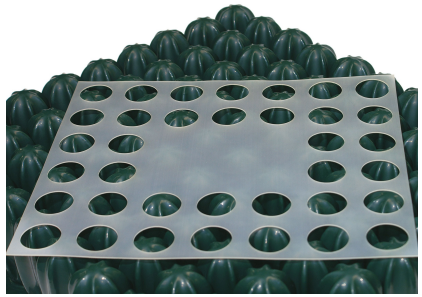

Coverplate

Cleaning and Maintenance

The use of the Conform cushion cover is recommended with the Conform cushion. Both cover and cushion can be machine washed in a low wash program. The cover can be machine washed at 40°C. The cushion can be machine washed from 30°C - 40°C. Please ensure that the valves of the cushion are closed during this process.

Conform cushions are salt-water resistant.

The cushion is made of natural rubber and it should be not be exposed to sunlight (UV-light), which could result in premature ageing of the material.

The requirement for storage, cleaning and maintenance are in accordance with DIN 7716.

Warranty

Conform cushions have a manufacturing warranty of 2 years.